

Gel Mark Breast Tissue Marker Family

Gel Mark Ultra™ Breast Tissue Markers



- 7G and 10G needles compatible with EnCor™ probes
- Ten (10) PLA/PGA pads provide 4-6 weeks of ultrasound visibility
- Stainless steel and titanium markers



Gel Mark UltraCor™ Breast Tissue Markers



- 14G rigid needle with beveled tip
- Four (4) PLA/PGA pads provide 4-6 weeks of ultrasound visibility
- Stainless steel and titanium markers



SenoMark Breast Tissue Marker Family

SenoMark™ Breast Tissue Markers



- 7G, 9G, 10G, 11G, and 12G needles compatible with EnCor™, ATEC™, Eviva™, and Mammotome™ probes
- Three (3) PGA pads provide 3 weeks of ultrasound visibility
- Stainless steel and titanium markers



SenoMark™ Ultra Breast Tissue Markers



- 7G, 9G, 10G, 11G, and 12G needles compatible with EnCor™, ATEC™, Eviva™, and Mammotome™ probes
- Three (3) PGA pads designed to assist in accurate placement and minimize migration, and one (1) PVA polymer for permanent ultrasound visibility
- BioDur™ 108 and titanium markers



SenoMark™ UltraCor™ Breast Tissue Markers



- 14G rigid needle with beveled tip
- PGA pads designed to assist in accurate placement and minimize migration, and one (1) PVA polymer provides permanent ultrasound visibility
- BioDur™ 108 and titanium markers



SenoMark™ UltraCor™ MRI Breast Tissue Markers



- 14G rigid needle with beveled tip
- Three (3) PGA pads for 13 cm needle provide 3 weeks of ultrasound visibility
- Stainless steel and titanium markers



INDICATIONS FOR USE:

The Gel Mark Ultra™, Gel Mark UltraCor™, StarchMark™, and StarchMark™ UltraCor™ Breast Tissue Markers are intended to radiographically mark breast tissue during a percutaneous breast biopsy procedure. The SenoMark™, SenoMark™ Ultra, and SenoMark™ UltraCor™ Breast Tissue Markers are intended to radiographically and sonographically mark breast tissue during a percutaneous breast biopsy procedure. The SenoMark™ UltraCor™ MRI Breast Tissue Marker is intended to radiographically and sonographically mark breast tissue prior to or during a percutaneous breast biopsy procedure. The UltraCor™ 17G Tissue Marker is indicated for use to radiographically mark breast tissue during a percutaneous breast biopsy procedure. The UltraClip™ and UltraClip™ Dual Trigger Breast Tissue Markers are intended for use to attach to soft breast tissue at the surgical site during an open surgical breast biopsy or a percutaneous breast biopsy to radiographically mark the location of the biopsy procedure. The UltraCor™ Twirl™ Breast Tissue Marker is intended for use to attach to soft breast tissue, including axillary lymph nodes, to radiographically mark the location of the biopsy procedure.

CONTRAINDICATIONS: Do not use this device in patients with a known hypersensitivity to the materials listed in the device description as they may suffer an allergic reaction to this implant. UltraCor™ Twirl™ Breast Tissue Marker only. The implant is made from a nickel-titanium alloy; if there is a known allergy to nickel, use of the UltraCor™ Twirl™ Breast Tissue Marker is not advised.

WARNINGS: Use caution when inserting near a breast implant to avoid puncture of the implant capsule. As with any foreign object implanted into the body, potential adverse reactions are possible. It is the responsibility of the physician to evaluate the risk/benefit prior to the use of this device. Bard™ Breast Tissue Markers have been designed for single use only. Reusing these medical devices bears the risk of cross-patient contamination as medical devices – particularly those with long and small lumina, joints,

and/or crevices between components – are difficult or impossible to clean once body fluids or tissues with potential pyrogenic or microbial contamination have had contact with the medical device for an indeterminate period of time. The residue of biological material can promote the contamination of the device with pyrogens or microorganisms which may lead to infectious complications. Do not resterilize. After resterilization, the sterility of the product is not guaranteed because of an indeterminate degree of potential pyrogenic or microbial contamination which may lead to infectious complications. Cleaning, reprocessing and/or resterilization of the present medical device increases the probability that the device will malfunction due to potential adverse effects on components that are influenced by thermal and/or mechanical changes. UltraCor™ and UltraCor™ Twirl™ Breast Tissue Markers only. The UltraCor™ and UltraCor™ Twirl™ Breast Tissue Markers are not recommended for use in patients with breast implants.

PRECAUTIONS: Breast Tissue Markers should only be used by a physician who is completely familiar with the indications, contraindications, limitations, typical findings and possible side effects of tissue marker placement. After use, the product may be a potential biohazard. Handle and dispose of in accordance with acceptable medical practice and applicable local laws and regulations. StarchMark™ and StarchMark™ UltraCor™ Breast Tissue Markers only. Although polysaccharide (starch) has known hemostatic properties, the user should continue to employ standard methods for obtaining hemostasis following the biopsy procedure.

COMPLICATIONS: Complications may occur at any time during or after the procedure. Potential complications of breast tissue marker placement may include, but are not limited to: hematoma, hemorrhage, infection, adjacent tissue injury and pain. Please consult product labels and inserts for complete indications, contraindications, hazards, warnings, precautions and directions for use.



An impressive line-up

With a variety of breast tissue marker options from BD, you can choose one that's right for her.

BD Switzerland Sarl
Terre Bonne Park – A4, Route De Crassier, 17, 1262 Eysins, Vaud, Switzerland
T: +41 21 556 3000



bd.com


Bard is now a wholly owned subsidiary of BD BD, the BD Logo and all other trademarks are the property of Becton, Dickinson and Company. © 2021 BD and its subsidiaries. All rights reserved. 0621/6132 BD-29895



An exceptional choice of breast tissue markers

Designed for accurate placement, minimal migration, and clear visibility in a variety of modalities. Choose from 13 breast tissue marker shapes:

Shapes

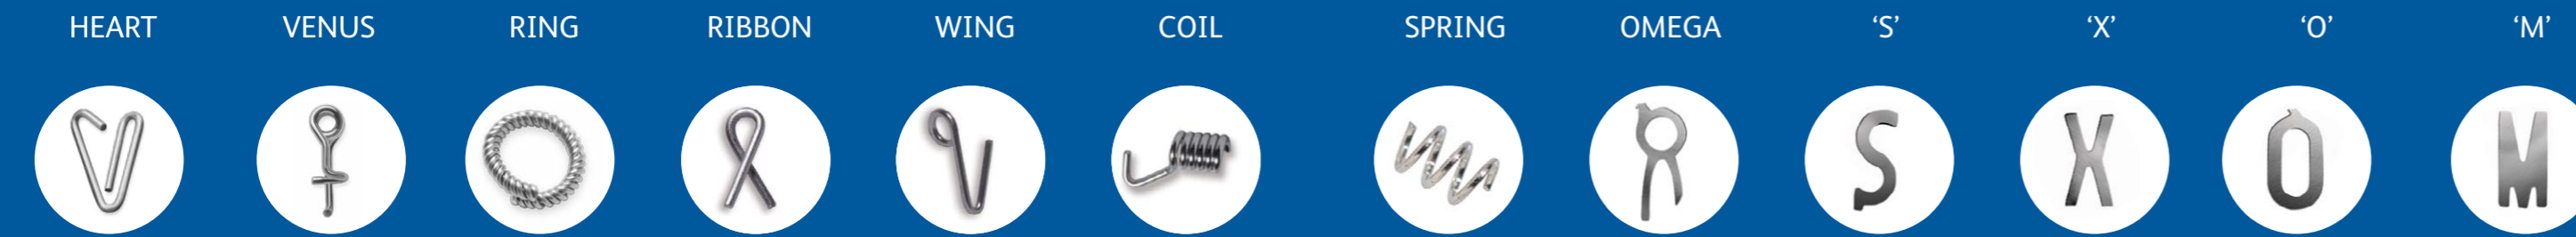

Markers

Titanium	BioDur™ 108	Nitinol	Titanium	Inconel™ 108	BioDur™ 108	Stainless steel	Stainless steel	Titanium	Titanium	Titanium	Stainless steel
SenoMark™ UltraCor™ Breast Tissue Marker	UltraClip™ Dual Trigger Breast Tissue Marker	UltraCor™ Twirl™ Breast Tissue Marker	SenoMark™ Ultra Breast Tissue Marker	UltraClip™ Breast Tissue Marker	SenoMark™ Ultra Breast Tissue Marker	UltraClip™ Breast Tissue Marker	Gel Mark Ultra™ Breast Tissue Marker	Gel Mark UltraCor™ Breast Tissue Marker	SenoMark™ Breast Tissue Marker	SenoMark™ Breast Tissue Marker	SenoMark™ Breast Tissue Marker
UltraClip™ Dual Trigger Breast Tissue Marker	SenoMark™ UltraCor™ Breast Tissue Marker	UltraClip™ Breast Tissue Marker	UltraClip™ Breast Tissue Marker	UltraClip™ Breast Tissue Marker	UltraClip™ Breast Tissue Marker	UltraClip™ Breast Tissue Marker	Gel Mark UltraCor™ Breast Tissue Marker	SenoMark™ Breast Tissue Marker	SenoMark™ UltraCor™ MRI Breast Tissue Marker	SenoMark™ UltraCor™ MRI Breast Tissue Marker	SenoMark™ UltraCor™ MRI Breast Tissue Marker
		UltraClip™ Dual Trigger Breast Tissue Marker		UltraClip™ Dual Trigger Breast Tissue Marker			SenoMark™ Breast Tissue Marker				

Visualisations



Options to fit your needs -

More choices for you and for her.

UltraClip™ Breast Tissue Marker Family

UltraClip™ Dual Trigger Breast Tissue Markers



- 17G rigid needle with beveled tip
- One (1) PVA polymer for permanent ultrasound visibility
- Inconel™ 625, BioDur™ 108, and titanium markers

UltraClip™ Breast Tissue Markers



- 17G rigid needle with beveled tip
- Safety switch that helps prevent premature deployment of marker
- Inconel™ 625, BioDur™ 108, and titanium markers

UltraCor™ Breast Tissue Marker Family

UltraCor™ Breast Tissue Markers



- 17G rigid needle with beveled tip
- Two (2) PEG plugs in distal and proximal positions
- Stainless steel marker

UltraCor™ Twirl™ Breast Tissue Markers



- 17G rigid needle with beveled tip
- Polymer and gel-free to limit materials in breast and axillary lymph nodes
- Nitinol marker
- Indicated for axillary lymph nodes and breast tissue